


# MIC Test Strip

Quantitative assay for determining the Minimum Inhibitory Concentration (M.I.C.)

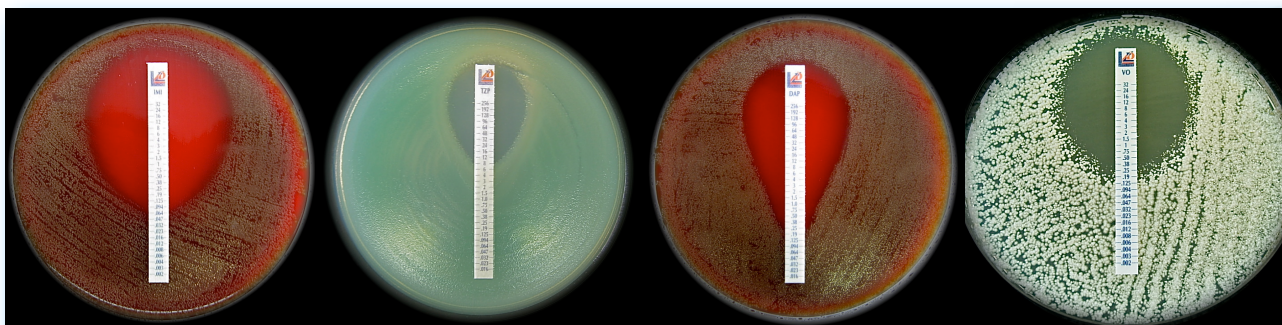


*S. pneumoniae* ATCC® 49619  
IMIPENEM 0.002-32 µg/mL  
M.I.C. = 0.094 µg/mL

*P. aeruginosa* ATCC® 27853  
PIPE,-TAZO. 0.016-256 µg/mL  
M.I.C. = 8 µg/mL

*S. pneumoniae* ATCC® 49619  
DAPTOMYCIN 0.016-256 µg/mL  
M.I.C. = 0.25 µg/mL

*C. krusei* ATCC® 6258  
VORICONAZOLE 0.002-32 µg/mL  
M.I.C. = 0.25 µg/mL

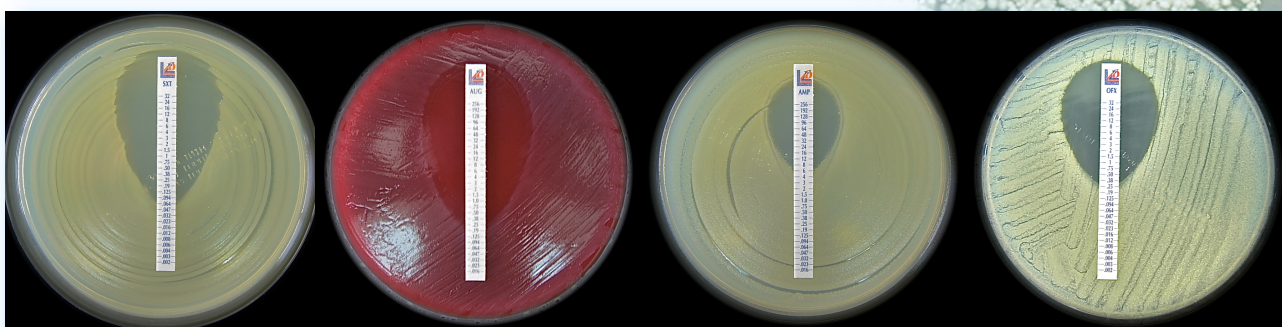


*E. coli* ATCC® 25922  
TRIMET.-SULFAM. 0.002-32 µg/mL  
M.I.C. = 0.094 µg/mL

*B. fragilis* ATCC® 25285  
AM.-CLAV. Ac. (2/1) 0.016-256 µg/mL  
M.I.C. = 0.25 µg/mL

*E. coli* ATCC® 25922  
AMPICILLIN 0.016-256 µg/mL  
M.I.C. = 8 µg/mL

*S. aureus* ATCC® 29213  
OFLOXACIN 0.002-32 µg/mL  
M.I.C. = 0.38 µg/mL

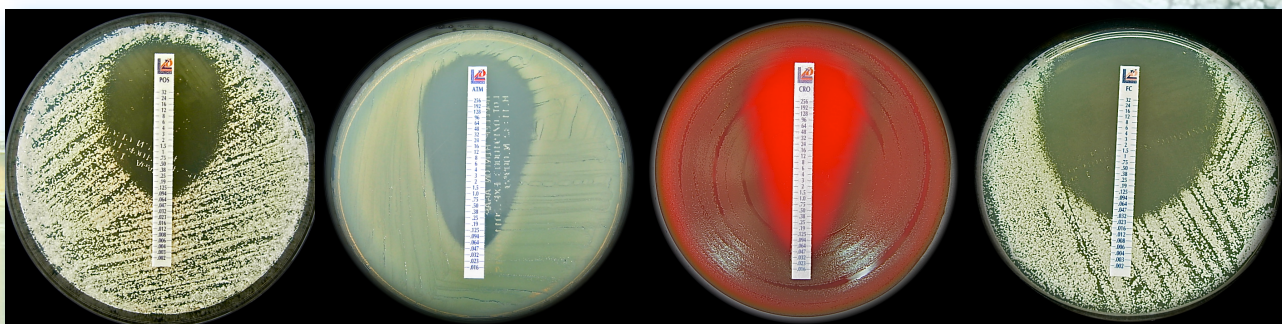


*C. krusei* ATCC® 6258  
POSACONAZOLE 0.002-32 µg/mL  
M.I.C. = 0.094 µg/mL

*E. coli* ATCC® 25922  
AZTREONAM 0.016-256 µg/mL  
M.I.C. = 0.064 µg/mL

*S. pneumoniae* ATCC® 49619  
CEFTRIAXONE 0.016-256 µg/mL  
M.I.C. = 0.064 µg/mL

*C. tropicalis* ATCC® 750  
FLUCYTOSINE 0.002-32 µg/mL  
M.I.C. = 0.032 µg/mL

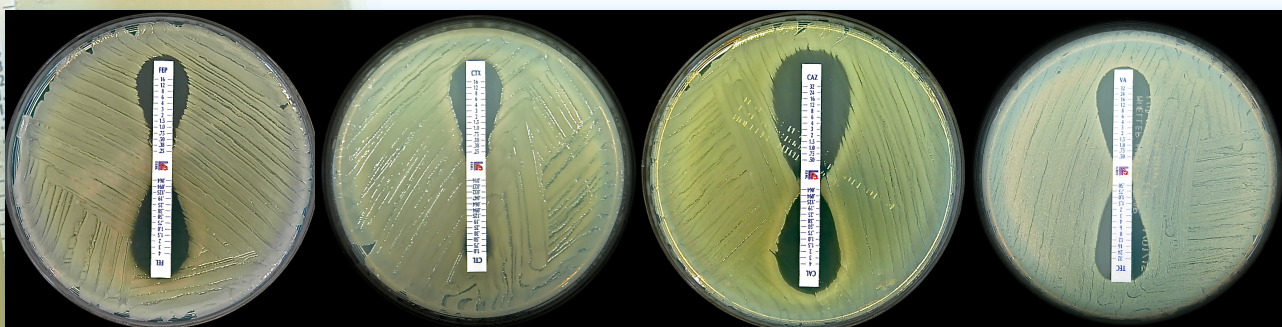

*K. pneumoniae* ATCC® 700603  
FEP/FEL 0.25-16/0.064-4 µg/mL  
M.I.C. FEP = ellipse deformation  
M.I.C. FEL = 0.094 µg/mL

*K. pneumoniae* ATCC® 700603  
CTX/CTL 0.25-16/0.016-1 µg/mL  
M.I.C. CTX = ellipse deformation  
M.I.C. CTL = 0.5 µg/mL

*E. coli* ATCC® 25922  
CAZ/CAL 0.5-32/0.064-4 µg/mL  
M.I.C. CAZ < 0.5 µg/mL  
M.I.C. CAL = 0.094 µg/mL

*S. aureus* ATCC® 29213  
VANCO./TEICOP. 0.5-32/0.5-32 µg/mL  
M.I.C. VA = 0.5 µg/mL  
M.I.C. TEC = 1 µg/mL



Liofilchem® s.r.l.

Via Scozia zona ind.le, 64026 Roseto degli Abruzzi (Te) Italy

Tel. +39 0858930745

Fax +39 0858930330

www.liofilchem.net

liofilchem@liofilchem.net



MIC Test Strip  
patent pending